

The Research of a New Iteration of the Circular Algorithm

Xu Shuping

School of Computer Science and Engineering
Xi'an Technological University
Xi'an, 710021, China
e-mail: 563937848@qq.com

Chen Li

School of Computer Science and Engineering
Xi'an Technological University
Xi'an, 710021, China

Huang Menyao

School of Computer Science and Engineering
Xi'an Technological University
Xi'an, 710021, China

Xu Pei

School of Computer Science and Engineering
Xi'an Technological University
Xi'an, 710021, China

Abstract—It is a problem of spectra analysis of flue gas that how to separate and calculate the concentration of different kinds of gas from continuous mixed gas absorption spectrum signal. So based on experimental data, a new iteration of the circular algorithm is put forward on the basis of Lambert-Beer's law. The algorithm uses different UV-light wavelengths at 190nm-290nm for different characteristics of UV light with different absorption peaks. The iteration is repeated until the concentration difference between adjacent two gases is less than a certain value. It is considered that the elemental gas The exact concentration, and through the programming to achieve the results. it has strong anti-jamming capability and is suitable for practical application of engineering.

Keywords—Circular Iteration; Characteristic Absorption Peak; Iterative Algorithm; Gas Concentration

I. INTRODUCTION

With the industrial production, centralized heating of boilers and the popularization of transportation tools, a large number of soot and toxic and harmful gases will be discharged. Hazardous substances accumulate gradually in the atmosphere and reach a certain concentration, which will make the normal composition of air change, thus endangering the health of human beings and various animals and plants. Various problems caused by air pollution have attracted the attention of environmental protection departments. In order to achieve accurate and real-time monitoring of environmental quality, ecological environment and pollution sources, and provide accurate basis for supervision and management of environmental protection departments at all levels and

environmental decision-making of the government, a large number of modern environmental monitoring instruments are urgently needed.

At present, there are three main methods for gas detection of portable spectrometers in domestic and foreign markets: differential algorithm, electrochemical analysis and infrared spectroscopy. Differential absorption algorithm can accurately calculate the concentration of most gases, but it will lose the broadband continuous absorption information in the characteristic absorption of gases, leading to some gas concentration measurement can not come out. For example, the absorption spectrum of nitrogen dioxide molecule in the ultraviolet band is mostly gradual continuous absorption, so differential absorption algorithm may think that the absorption information of nitrogen dioxide is filtered out by scattering, resulting in the detection of nitrogen dioxide. If the absorption curves of nitric oxide and nitrogen dioxide have the same absorption peaks, the fitting absorption curves are superimposed at the measuring points, so it is still impossible to distinguish the two gases. The electrochemical analysis method has the advantages of simple structure and easy operation. It mainly depends on gas sensors, a gas sensor can only detect a corresponding gas, and the sensitivity of gas sensors is high, but after a period of time, the sensitivity of sensors to gas will decline, it is necessary to replace gas sensors in time, and gas sensors are expensive, which increases the use cost for users. The main principle of gas sensor is to use the oxidation or reduction reaction of gas to generate current, but if there are both oxidizing gas and reducing gas, the measurement results will be inaccurate. Infrared spectroscopy overcomes the shortcomings of

electrochemical analysis, but can only measure the approximate concentration of nitrogen oxides, can not accurately measure the specific concentration of NO and NO₂, and infrared spectroscopy for environmental humidity, temperature and other external conditions require higher technology is more complex .

Based on defects and deficiencies of the above gas detection methods, an iterative evolution gas solution algorithm is proposed in this paper. According to the good absorption of ultraviolet light by gas at the wavelength of 190-290 nm, the number of absorbed photons can be obtained by measuring the ultraviolet light absorbed by gas. The actual concentration of gas can be obtained from the number of photons by using the iterative gas calculation algorithm.

II. THE PINCIPLE AND COMPUTATIONAL PROCEDURE OF ITERATIVE ALGORITHMS

A. Algorithm Principle

Mixed gases have characteristic absorption peaks in the range of ultraviolet wavelength 190-290 nm. Gas absorbance has multiple superposition. Assuming that some elementary gas does not absorb other gases on its best characteristic absorption peak, the corresponding table of absorbance and concentration of this single substance gas is searched to obtain the initial concentration of the gas, and then switch to another characteristic absorption peak. The photon number of the gas is subtracted from the total photon number measured, and the initial concentration of another gas is obtained. By analogy, the initial concentration of each gas is obtained one by one. Then, the characteristic absorption peak of the first gas is returned to, and the absorption photon number of other gases is subtracted from the total photon number absorbed, and the iterative concentration of the first gas is obtained again. By analogy, the initial concentration of each elemental gas is obtained again. By repeating the iteration until the difference of gas concentration between two adjacent times is less than a certain value, it is considered that the concentration of the elemental gas is obtained.

B. Algorithm Steps

1) The initial concentration c_1 of the first elementary gas in the mixed gas is solved. According to the characteristic absorption peak of the gas at wavelength λ_1 , the number of photons $B S_{\lambda_1}$ absorbed by the gas is read. Solving the value of $\frac{R_{\lambda_1} - D_{\lambda_1}}{S_{\lambda_1} - D_{\lambda_1}}$ (R_{λ_1} is the number of incident photons; S_{λ_1} is the number of photons passing through the

medium.; D_{λ_1} is the number of photons in dark spectrum(Also known as dark spectral noise); λ_1 is the wavelength of a certain ultraviolet wave, K is a constant, c is the concentration of elemental gas), The initial concentration c_1 of the elemental gas was obtained by inquiring the comparison table of absorbance and gas concentration..

2) The initial concentration c_2 of the second primary gas in the mixed gas is solved. too, Select the characteristic absorption peak λ_2 of the elemental gas and read the absorption photon number S_{λ_2} of the elemental gas. Assuming that there are only two gases in this band, According to the formula

$$\frac{R_{\lambda} - D_{\lambda}}{S_{\lambda} - D_{\lambda}} = \frac{R_{\lambda_1} - D_{\lambda_1}}{S_{\lambda_1} - D_{\lambda_1}} * \frac{R_{\lambda_2} - D_{\lambda_2}}{S_{\lambda_2} - D_{\lambda_2}} \quad (1)$$

the absorbance of the second gas is calculated, and the concentration of the second gas is calculated by querying the absorbance and concentration table again, as the initial concentration c_2 of the second gas.

3) Solve the concentration of other elemental gases in mixed gases. Methods 1 and 2. Selecting the characteristic peak absorption wavelength of other elemental gases and reading the number of absorbed photons at that wavelength. The absorbance was calculated by formula

$$A = \frac{R_{\lambda} - D_{\lambda}}{S_{\lambda} - D_{\lambda}} = \frac{R_{\lambda_1} - D_{\lambda_1}}{S_{\lambda_1} - D_{\lambda_1}} * \frac{R_{\lambda_2} - D_{\lambda_2}}{S_{\lambda_2} - D_{\lambda_2}} * \frac{R_{\lambda_3} - D_{\lambda_3}}{S_{\lambda_3} - D_{\lambda_3}} * \dots * \frac{R_{\lambda_n} - D_{\lambda_n}}{S_{\lambda_n} - D_{\lambda_n}} \quad (2)$$

(A is absorbance), and the initial concentration of gas was obtained by looking up the table.

4) Iterative Recursion of the Concentration of the First Element Gas. The concentration of all elemental gases obtained at present is substituted into the formula

$$\frac{R_{\lambda} - D_{\lambda}}{S_{\lambda} - D_{\lambda}} = \frac{R_{\lambda_1} - D_{\lambda_1}}{S_{\lambda_1} - D_{\lambda_1}} * \frac{R_{\lambda_2} - D_{\lambda_2}}{S_{\lambda_2} - D_{\lambda_2}} * \frac{R_{\lambda_3} - D_{\lambda_3}}{S_{\lambda_3} - D_{\lambda_3}} * \dots * \frac{R_{\lambda_n} - D_{\lambda_n}}{S_{\lambda_n} - D_{\lambda_n}} \quad (3)$$

and the corresponding S_{λ_1} of wavelength λ_1 is read again. The iterative concentration c_1 of the first elemental gas is obtained by checking the corresponding table of concentration absorbance.

5) Repeat 2) and 3) to find the iteration concentration c_{m1} of the elemental gas M.

6) Calculate the error of the calculation results of the same elemental gas in the adjacent two times. The first-order iteration error of each elemental gas is calculated.

$$\Delta_{m1} = |c_{0m} - c_{m1}| \tag{4}$$

7) Repeat 4, 5 and 6 until the error of two iterations of the same gas concentration is less than 3%.

$$\Delta_n < \Delta_G \tag{5}$$

The last calculated gas concentration is regarded as the final concentration of various elemental gases.

III. ALGORITHM VERIFICATION

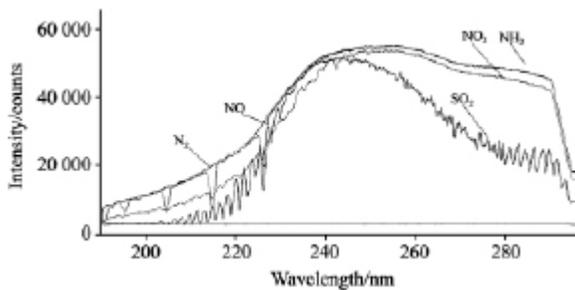


Figure 1. Mixed gas UV spectral absorption curve

Fig.1 is the absorption spectra of NO , SO_2 , NH_3 and NO_2 mixed gases. Among them, N_2 is a zero gas whose spectral line is called zero gas line. Zero gas is not absorbed in ultraviolet light of 190-290 nm. Because there is Rayleigh scattering in the gas to be detected, the influence of scattering can be eliminated by using the zero-gas line spectrum as the reference spectrum.

From the observation in Fig.1, we can see that NO and NH_3 can find non-interference absorption wavelengths. These two wavelengths are just the absorption peaks of NO and NH_3 , and there is no NO absorption at the NH_3 absorption peak, and there is no NH_3 absorption at the NO absorption peak. So it is easy to distinguish the two gases if we only distinguish them. The problem now is that SO_2 and NO_2 both absorb at the absorption peaks of these two gases. At the wavelength of 220 nm, the maximum absorption peaks of NO and NO_2 are close, and

SO_2 absorbs a lot of ultraviolet light in this section. So if we can know the concentration of SO_2 and NO_2 beforehand, we can use the superposition of absorbance to subtract the absorbance of NO and NH_3 from the total absorbance of SO_2 and NO_2 . We can get the absorbance of NO and NH_3 by looking up tables. Therefore, in order to obtain the specific concentration of various elemental gases in mixed gases, the concentration of SO_2 and NO_2 must be required first, and then the concentration of NO and NH_3 can be calculated. In this way, the concentration of four kinds of elemental gases in the mixture can be calculated.

A. Calculating the Concentrations of SO_2 and NO_2

NO_2 and SO_2 interfere with each other in the whole working band. Now it is assumed that there are two kinds of elemental gases in the mixture, NO_2 and SO_2 , respectively. It is now known that the absorption spectra of mixed gases at 231.33 nm and 273.33 nm, and the absorbance of gases NO_2 and SO_2 at 231.33 nm and 273.33 nm (231.33 nm and 273.33 nm, respectively, are the maximum absorbance of gases NO_2 and SO_2 at this point). Now calculate the respective concentrations of NO_2 and SO_2 .

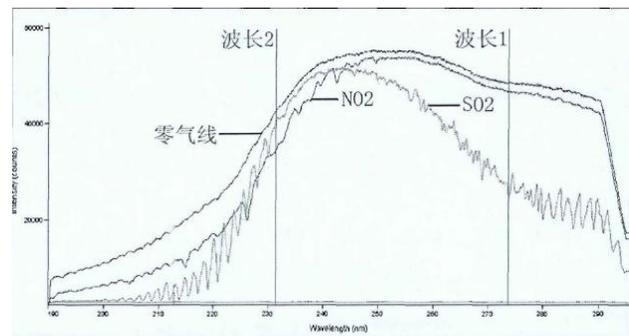


Figure 2. Absorption spectra of SO_2 and NO_2

TABLE I. SPECTRAL TABLES FOR SO_2 AND NO_2 AT WAVELENGTH 273.33NM AND WAVELENGTH 231.33NM

Wavelength	231.33	273.33
NO_2 absorbance	0.03003444	0.00456189
SO_2 absorbance	0.00482312	0.07984884

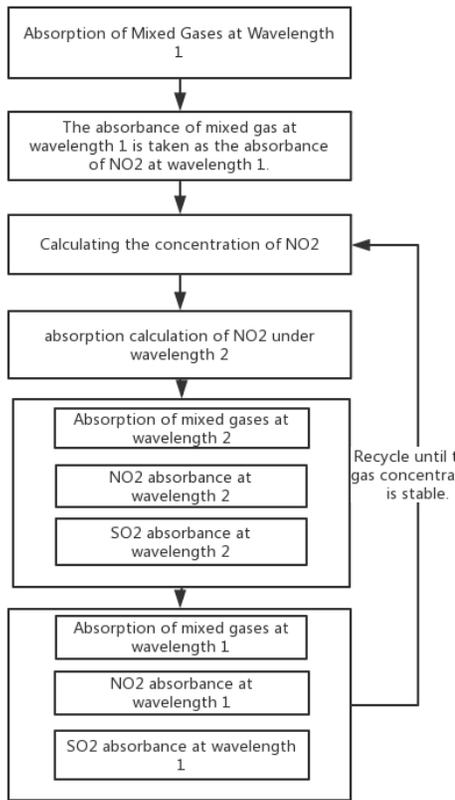


Figure 3. NO₂ and SO₂ gas concentration iterative algorithm flow chart

Fig. 3 is the flow chart of the iterative algorithm for the concentration of NO₂ and SO₂ mixed gases. After several iterations, the real concentrations of these two gases can be calculated from the mixture.

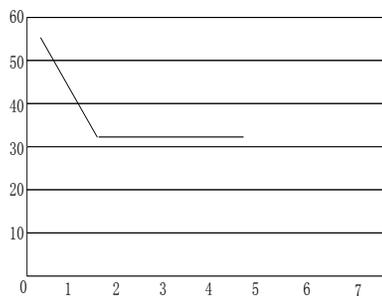


Figure 4. SO₂ concentration and the number of iterations curve

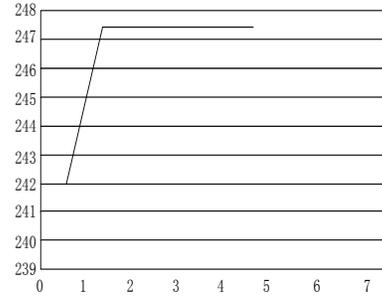


Figure 5. NO₂ concentration and the number of iterations curve

After two iterations, the numerical value of the algorithm tends to be stable, and the precise gas concentrations of NO₂ and SO₂ are basically obtained.

B. Calculating the Gas Concentrations of NO and NH₃

There is no interference between NO and NH₃ at their maximum absorption peaks, so the total absorbance and the concentration of NO₂ and SO₂ can be calculated according to the superposition of ultraviolet light. Assuming that the concentrations of NO₂ and SO₂ in mixed gases are c₁ and c₂, respectively, and the concentrations of NO and NH₃ are c₃ and c₄, the multivariate superposition of absorbance at wavelength 225.88 nm can be obtained as follows:

$$A = A_1 + A_2 + A_3 \tag{6}$$

A₁ is the absorbance of NO₂ at 225.8 nm in c₁ concentration, A₂ is the absorbance of SO₂ at 225.8 nm in c₂ concentration, A is the total absorbance of mixed gas at 225.88 nm and A₃ is the total absorbance of NO at 225.88 nm.

$$A_3 = A - A_1 - A_2 = \lg\left(\frac{I_0}{I}\right) - A_1 - A_2 \tag{7}$$

I₀ is the spectral intensity at 225.88 nm through zero gas, I is the transmission intensity at 225.88 nm through the mixture gas to be measured, the intensity can be obtained directly by spectrometer, A₂ and A₃ are calculated by the concentration of SO₂ and NO₂. In this way, the absorbance A₃ of NO at 225.88 nm can be obtained, and then the concentration of NO can be calculated according to the corresponding table between the concentration of NO at 225.88 nm and the absorbance. The absorbance

A_4 of NH_3 can be obtained by the same method at 208.23 nm, and the concentration of NH_3 can be calculated according to the corresponding relationship between NH_3 concentration and absorbance at 208.23 nm.

C. Composition of Platform Experiment System

Ultraviolet flue gas analyzer consists of three parts: flue gas data acquisition module, data processing module and data display module.

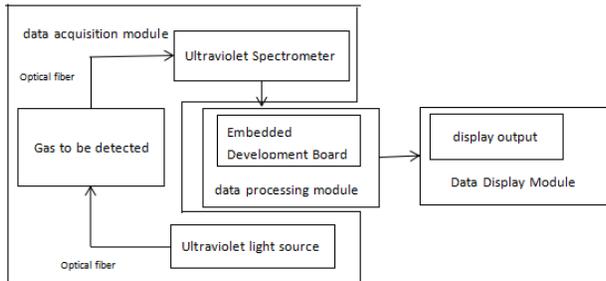


Figure 6. Experimental system composition diagram

The data acquisition module is composed of ultraviolet light source and marine optical Maya2000 Pro ultraviolet spectrometer. Ultraviolet light source outputs stable ultraviolet light. Ultraviolet light passes through the optical fiber through the detected gas. After the gas is fully absorbed, the remaining ultraviolet light is transmitted into the ultraviolet spectrometer by the optical fiber. After the optical processing and photoelectric conversion of the gas by the spectrometer, the gas information becomes an electrical signal, waiting for the data processing module to read. In this system, the ultraviolet spectrometer is actually a flue gas acquisition sensor. Data processing module is composed of embedded development board. The embedded development board reads the gas information from the ultraviolet spectrometer, calculates the actual concentration of the elemental gas through the iterative algorithm, and visualizes it through the data display module. This is the composition and working principle of the experimental system.

D. Absorption Spectroscopy of Elemental Gas and Zero Gas

N_2 is introduced into the system, and its absorption spectrum is measured when the gas concentration is stable. After that, the number of photons absorbed by NO_2 , NO , SO_2 and NH_3 gases was measured in turn, and the curve was drawn by using the number and wavelength of photons.

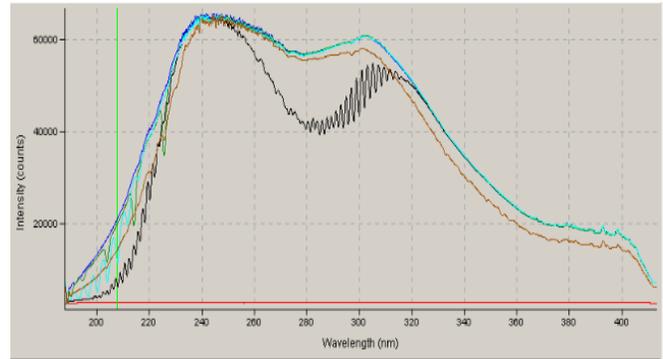


Figure 7. Four gas photon spectrum line graph

E. Data Verification

The following data are obtained when a mixture of SO_2 and NO is injected into the experimental system.

TABLE II. 200 PPM SO_2 AND NO GAS SPECTRAL DATA

	271.98nm	225.94nm	dark noise
zero gas	56434	43973	2900
SO_2 100ppm	52851	42754	2900
zero gas	56434	43973	2900
NO_2 100ppm	56386	40749	2900

Table 2 shows the number of absorbed photons and dark noise photons at 271.98 and 225.94 nm measured by ultraviolet spectrometer in a mixture of SO_2 and NO_2 at 100 ppm, respectively.

TABLE III. SPECTRAL DATA FOR MIXED GAS

	271.98nm	225.94nm	dark noise
zero gas	56434	43973	2900
mixed gas	52050	39588	2900

Table 3 shows the number of absorbable photons at 271.98 nm and 225.94 nm for zero and mixed gases, as well as the number of dark spectral noise photons measured by spectrometer. In practical calculation, the number of photons measured should be subtracted from the number of photons of dark spectral noise to obtain the actual number of photons of zero gas and mixed gas.

Based on the above data, the photon number absorption curves of elemental gases at their maximum absorption peaks are fitted.

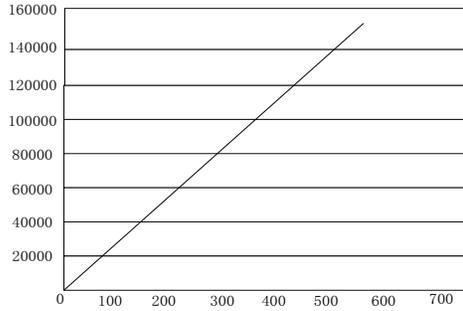


Figure 8. Fitting curve of SO₂ at 271.98 nm

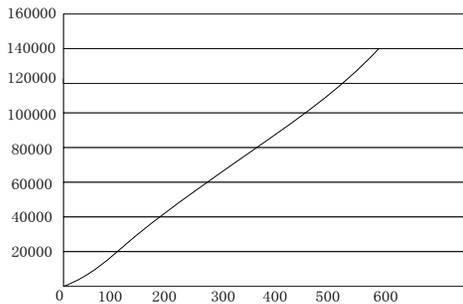


Figure 9. Fitting curve of NO at 225.94 nm

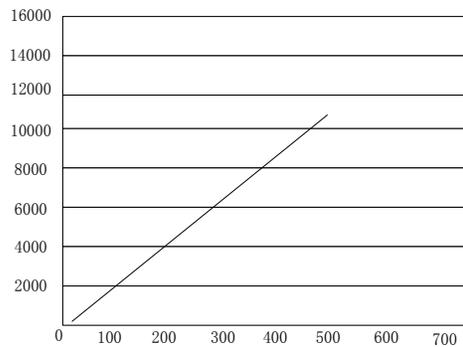


Figure 10. Fitting curve of NO at 271.98 nm

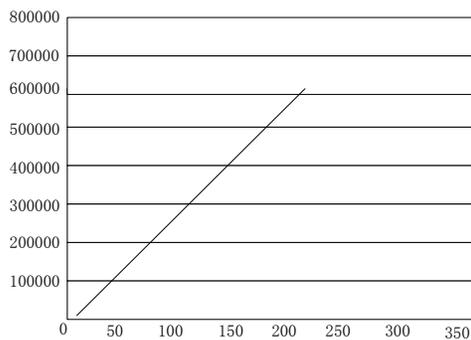


Figure 11. Fitting curve of NH₃ at 271.98 nm

Figure 8-11 is a curve drawn by a single gas at the maximum absorption wavelength of ultraviolet light. Analysis table of experimental results

TABLE IV. ANALYSIS OF RESULTS

gas species	standard value (ppm)	measured value (ppm)	difference value	maximum difference	error
SO ₂	102	104	2	-4	0.8%
	200	196	-4		
	499	501	2		
NO	104	108	4	-7	1.4%
	200	206	6		
	500	493	-7		
NO ₂	116	112	-4	-9.7	1.94%
	201.5	195	-6.5		
NH ₃	50	53	3	3	1.5%
	200	199	-1		
conclusion	Accuracy error is less than 3%, which meets the design standard.				

In Table 4, the standard value is the concentration of the standard elemental gas put in the test, and the measured value is the concentration of the elemental gas calculated from the mixed gas using an iterative algorithm. From the experimental results, it can be seen that the maximum error of the measured value is less than the standard value, and the maximum error of the accuracy is 1.94%, which is much less than the original design standard of 3%, which is within the normal standard.

IV. SOFTWARE IMPLEMENTATION

The software algorithm is written in JavaScript, including the analysis and implementation process of the iterative algorithm gas. The main code is as follows:

```

/*
 *Iterative calculation of gas concentration
 */
function GetGasC() {
 //1. Obtain absorbance from NO2
 var NO2A_1 = GetABByWa(gasWavebanc['NO2']);
 //2. Find the concentration of this point
 var NO2C_1, NO2A_2, SO2A_2, SO2C_2,
 SO2A_1, ONA_3, NH3A_4, ONC_3, NH3C_4;
 for(var i = 0; i < 2; i++) {
 NO2C_1=GetCByA_Data(NO2_data_231,
 NO2A_1);
 //3.Calculate the absorbance of NO2 at 273.33.
 //NO2A_2;
 NO2A_2= getABByC_Data(NO2_data_273,
 NO2C_1);

```

//4. Obtain the total absorbance of SO₂ in the optimum band and subtract the absorbance of NO₂ here.

```
SO2A_2=GetAByWa(gasWavebanc["SO2"])
-NO2A_2;
```

//5. Looking up Table to Find DeSO₂C₁

```
SO2C_2 = GetCByA_Data(SO2_data_273,
SO2A_2);
```

//6. The absorbance of SO₂ at 231.33 was obtained by //looking up the table.

```
SO2A_1 = getAByC_Data(SO2_data_231,
SO2C_2);
```

//7. NO₂A₁ is the total absorbance minus the //absorbance of SO₂A₁ at 231.33.

```
NO2A_1 = NO2A_1 - SO2A_1;
```

```
}
```

```
currentGasC_NO2 = NO2C_1;
```

```
currentGasC_SO2 = SO2C_2;
```

//The absorbance of NO at the optimum band is the //total absorbance S-SO₂ absorbance minus the //absorbance of NO₂.

```
ONA_3 = GetAByWa(gasWavebanc["NO"]) -
getAByC_Data(NO2_data_225, NO2C_1) -
getAByC_Data(SO2_data_225, SO2C_2);
```

//Concentration of NO obtained

```
currentGasC_NO = GetCByA_Data(NO_data_225,
ONA_3);
```

```
NH3A_4 = GetAByWa(gasWavebanc["NH3"]) -
getAByC_Data(NO2_data_208, NO2C_1) -
getAByC_Data(SO2_data_208, SO2C_2);
```

```
currentGasC_NH3
```

```
GetCByA_Data(NH3_data_208, NH3A_4);
```

```
$("#NO2_C").html("No2 " +
currentGasC_NO2);
```

```
$("#SO2_C").html("So2 " + currentGasC_SO2);
```

```
$("#NO_C").html("NO " + currentGasC_NO);
```

```
$("#NH3_C").html("NH3 " +
currentGasC_NH3);
```

```
}
```

V. CONCLUSION

Aiming at the detection requirement of main harmful components in air pollution, a fast iteration algorithm of mixed flue gas is designed by using the continuous frequency division method of ultraviolet grating in the experimental system, and the effectiveness of the algorithm is verified. Ultraviolet spectrometer is used as a sensor. The embedded development board reads and calculates the gas

concentration. The analysis and calculation of the algorithm are realized by programming. The results show that the iterative algorithm can accurately measure the concentration of flue gas and keep the error within 3%. It can meet the design requirements and solve many kinds of gases at the same time. It is suitable for practical engineering applications.

ACKNOWLEDGMENT

Thank you, Shaanxi Education Department. This work was supported in part by a grant from Shaanxi Provincial Department of Education Project (15JF019).

The authors wish to thank the cooperators. This research is partially funded by the Project funds in shanxi province department of education (15JF019), a the Project funds in engineering laboratory project (GSYSJ2018011) and the project funds in innovation and entrepreneurship training for college students (1070214033)

ABOUT THE AUTHOR

Xu Shuping (1974-), Female, Professor, School of Computer Science and Engineering, Xi'an Technological University, majoring in embedded and computer control. Email: 563937848@qq.com, Mobile: 13772148209.

REFERENCES

- [1] Chen Zhi-gang. Discussion on Experimental Application of Lambert-Beer Law[J]. Acta Metrologica Sinica. 2015(1)
- [2] Pop,Paul. Embedded systems design:Optimization challenges.Lecture Notes in ComputerScience, 2014, 35(24):16-20
- [3] Shi Bao-song Sun Shou-hong Zhang Wei. Application of CCD in the portable spectrometer[J]. Electronic Measurement Technology. 2016(11)
- [4] Limited ARM Development Guide 2000-2001.ARM DOI.2013.06.
- [5] Tang Qu. "Research and design of ultraviolet flue gas analyzer [J]". Nanjing University of Technology. 2013
- [6] Jiang Xuqian. "Design of portable ultraviolet flue gas analyzer [J]". Nanjing University of Technology. 2012
- [7] Chen Bin. "Design of ultraviolet flue gas analyzer [J]".Nanjing University of Technology. 2016
- [8] Juwu ,Wu Yihui. Micro-miniaturization of spectrometer [J]. Journal of Instrumentation, 2013, 22 (4): 131-133
- [9] Yu Zhiqiang, Wenzhi Yu, Xie Yingke, Zhou Suyi. The control system of multi-parameter water quality tester based on raspberry pie [J]. Instrumentation technology and Sensors, 2015 (06): 20-23.
- [10] Han Xiao, Wenzhi Yu, Xie Yingke, Wei Kanglin, Zhou Xiaofeng. Software design of control and signal processing system for multi-parameter water quality tester [J]. Instrumentation technology and Sensors, 2014 (08): 20-22